


HAZARDOUS LOCATION

CONTROL ROOM

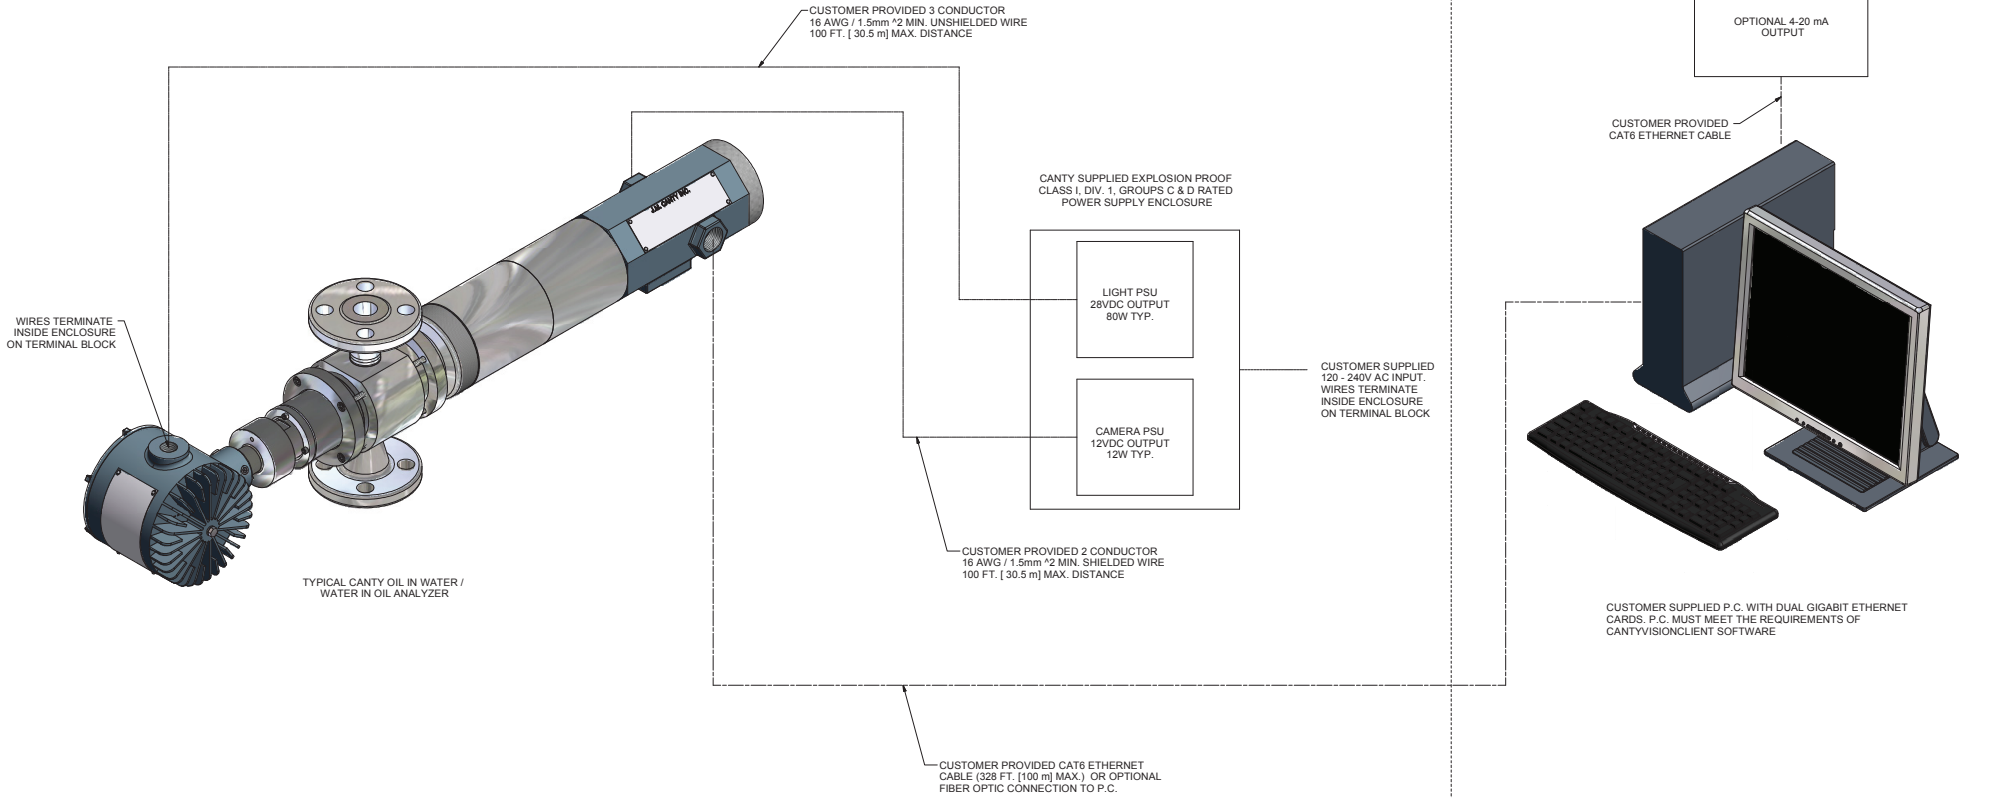

- NOTES:**
1. CABLE ENTRIES TO EXPLOSION PROOF POWER SUPPLY ENCLOSURE ARE 1- 11 1/2 NPT, 3X.
 2. CAMERA AND LIGHT SOURCE ARE BOTH SUPPLIED WITH M6 X 1.0 EXTERNAL EARTH CONNECTIONS, NOT SHOWN FOR SIMPLIFICATION.
 3. ETHERNET CAMERA IS PROVIDED WITH AN INTERNAL RJ-45 JACK FOR ETHERNET OUTPUT. INPUT POWER TO CAMERA IS PROVIDED WITH A 12" [30 CM] 2 CONDUCTOR PIGTAILED/FLYING LEAD INPUT POWER CONNECTION WITH REWIREABLE CONNECTOR. A MATING REWIREABLE CONNECTOR IS ALSO PROVIDED.
 4. ALL SYSTEMS ARE PROVIDED WITH OPC OUTPUT AT NO CHARGE. REF DOCUMENT TA10560-1. OPTIONAL 4-20 mA OUTPUT OPTION IS AVAILABLE. SEE DATASHEET TA9868-1 FOR PIN AND DETAILS.
 5. A DEDICATED NETWORK SEGMENT IS REQUIRED BETWEEN ETHERNET CAMERA AND CUSTOMER SUPPLIED P.C..
 6. OPTIONAL MOUNTING BRACKETS FOR EXPLOSION PROOF POWER SUPPLY ENCLOSURE ARE AVAILABLE.

<p>NOTICE THIS DRAWING IS THE PROPERTY OF J.M. CANTY AND MUST BE RETURNED WITHOUT REPRODUCTION OR DUPLICATION, AT ANY TIME UPON REQUEST, BUT IN ANY EVENT AS SOON AS IT HAS SERVED THE PURPOSE FOR WHICH IT WAS FURNISHED, WHILE IN THE POSSESSION OF THE RECIPIENT, IT MUST BE PROPERLY SAFEGUARDED AGAINST DISCLOSURE TO ANYONE EXCEPT THOSE EMPLOYEES WHO REQUIRE IT FOR WORK OR JOB. THE RECIPIENT MUST KEEP CONFIDENTIAL AND REQUIRE HIS (HER) EMPLOYEES TO KEEP CONFIDENTIAL THE INFORMATION CONTAINED HERE ON.</p>	<p>IMPORTANT FOR THE REQUIRED MANUFACTURING SPECIFICATIONS SEE DOCUMENT #A4955</p>	<p>DRAWN BY JD</p>	<p>DATE 8/11/2009</p>	<p>J.M. CANTY INC. 6100 DONNER RD. BUFFALO, N.Y. 14294 U.S.A.</p>	<p>CANTY WWW.JMCANTY.COM</p>	<p>J.M. CANTY INTL. LTD. BALLYCOOLIN BUS. PK. BLANCHARDSTOWN DUBLIN 15, IRELAND</p>
	<p>NOTE: FAILURE TO RECEIVE DOCUMENT DOES NOT WAIVE VENDOR RESPONSIBILITY</p>	<p>APPROVAL JD</p>	<p>DATE 8/11/2009</p>	<p>TITLE TYPICAL CABLE BLOCK DIAGRAM, OIL IN WATER / WATER IN OIL ANALYZER</p>		
	<p>ENGINEERING ANALYSIS CURRENT</p>	<p>DATE</p>	<p>FILE NAME TA11275-100</p>			
	<p>REVISIONS PENDING</p>	<p>DATE</p>	<p>SCALE AS NOTED</p>			
<p>QUALITY CONTROL I.O.A.</p>	<p>DATE</p>	<p>SHEET 1 OF 1</p>				